


## CERTIFIKÁTY ANALÝZY - MIC Test Stripy - Liofilchem s.r.l.

Certifikáty analýzy MIC Test stripů italského výrobce, společnosti Liofilchem, Itálie, které jsou specifické pro jednotlivé šarže výrobků, je možno si jednoduše stáhnout přímo z webových stránek výrobce.

### Postup stažení aktuálních certifikátů analýzy:

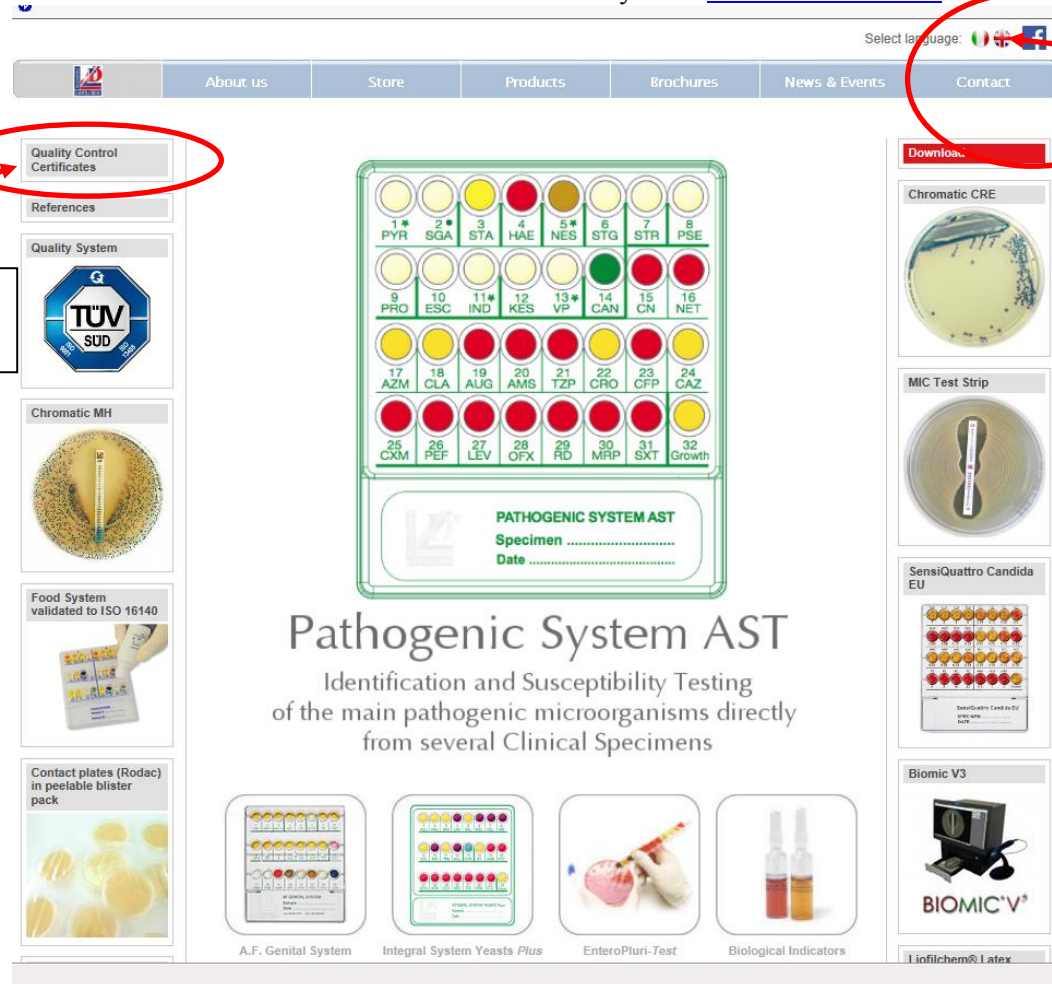


Otevřete webovou stránku výrobce [www.liofilchem.net](http://www.liofilchem.net)




The screenshot shows the Liofilchem website interface. At the top right, there is a 'Select language:' dropdown menu with flags for Italian, English, and Czech. A red circle highlights this menu, with an arrow pointing to a text box that says '1. KROK - Zvolte anglický jazyk'. On the left sidebar, there is a 'Quality Control Certificates' link, also highlighted with a red circle and arrow, pointing to a text box that says '2. KROK – Klikněte na ikonu Quality Control Certificates'. The main content area features a large image of a 'Pathogenic System AST' MIC test strip with 32 wells, each containing a different colored disc. Below the strip, the text reads 'Pathogenic System AST Identification and Susceptibility Testing of the main pathogenic microorganisms directly from several Clinical Specimens'. At the bottom, there are several smaller images of other Liofilchem products, including 'A.F. Genital System', 'Integral System Yeasts Plus', 'EnteroPluri-Test', 'Biological Indicators', 'Sensiquattro Candida EU', 'Biomic V3', and 'Liofilchem® Latex'.

1. KROK - Zvolte anglický jazyk

2. KROK – Klikněte na ikonu  
Quality Control Certificates

Select language:   

 [About us](#) [Store](#) [Products](#) [Brochures](#) [News & Events](#) [Contact](#)


### Quality Control Certificates

Enter the batch no. of the product:


**Quality Control Certificates**

**References**


**Quality System**




**Chromatic MH**



**Food System**  
Validated to ISO 16140




**Enteropluri-Test**




**Contact plates (Rodac)**

**Download**


**Chromatic CRE**




**MIC Test Strip**



**SensiQuattro Candida EU**






**Biomic V3**



**A.F. Genital System**

**Do okénka vložte POUZE číslo šarže výrobku bez katalogového čísla, např. 022714091**

**Klikněte na ikonu SEARCH**

Select language:   


[About us](#) [Store](#) [Products](#) [Brochures](#) [News & Events](#) [Contact](#)


### Quality Control Certificates


Enter the batch no. of the product:


[022714091-92147\\_921470\\_921471-02.2017.pdf](#)

**Download**

**Chromatic CRE**  


**MIC Test Strip**  



**SensiQuattro Candida EU**  



**Biomic V3**  
  
**BIOMIC V<sup>3</sup>**


**A.F. Genital System**


**Quality Control Certificates**


**References**

**Quality System**  


**Chromatic MH**  


**Food System validated to ISO 16140**  


**Enteropluri-Test**  


**Contact plates (Rodac)**  


**Zobrazí se odkaz umožňující stažení certifikátu analýzy dané šarže ve formátu pdf.**